

FIG. 1

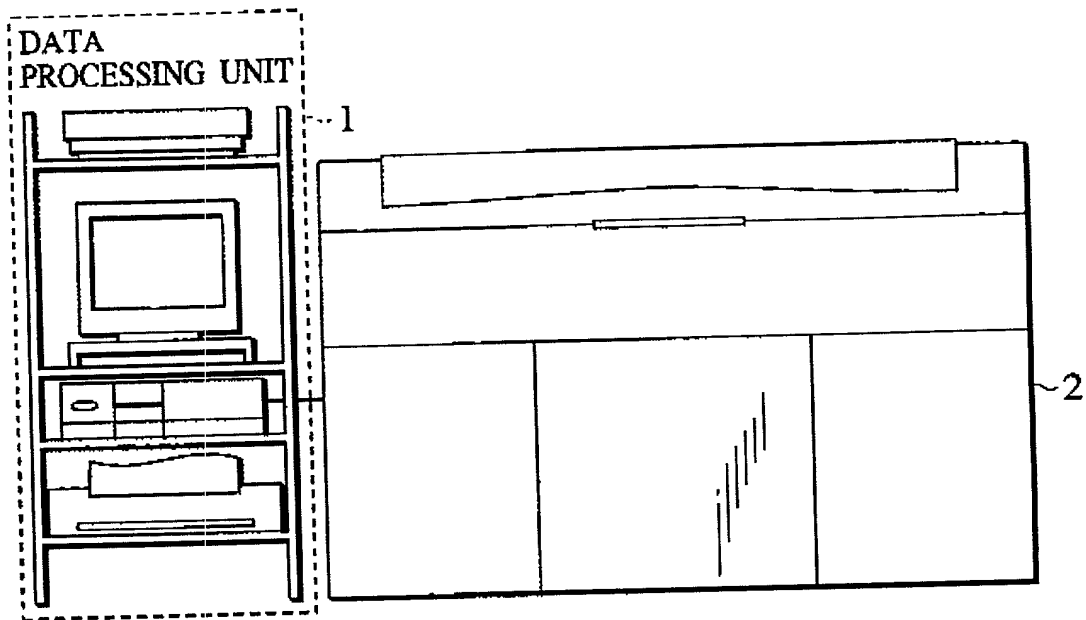


FIG. 2

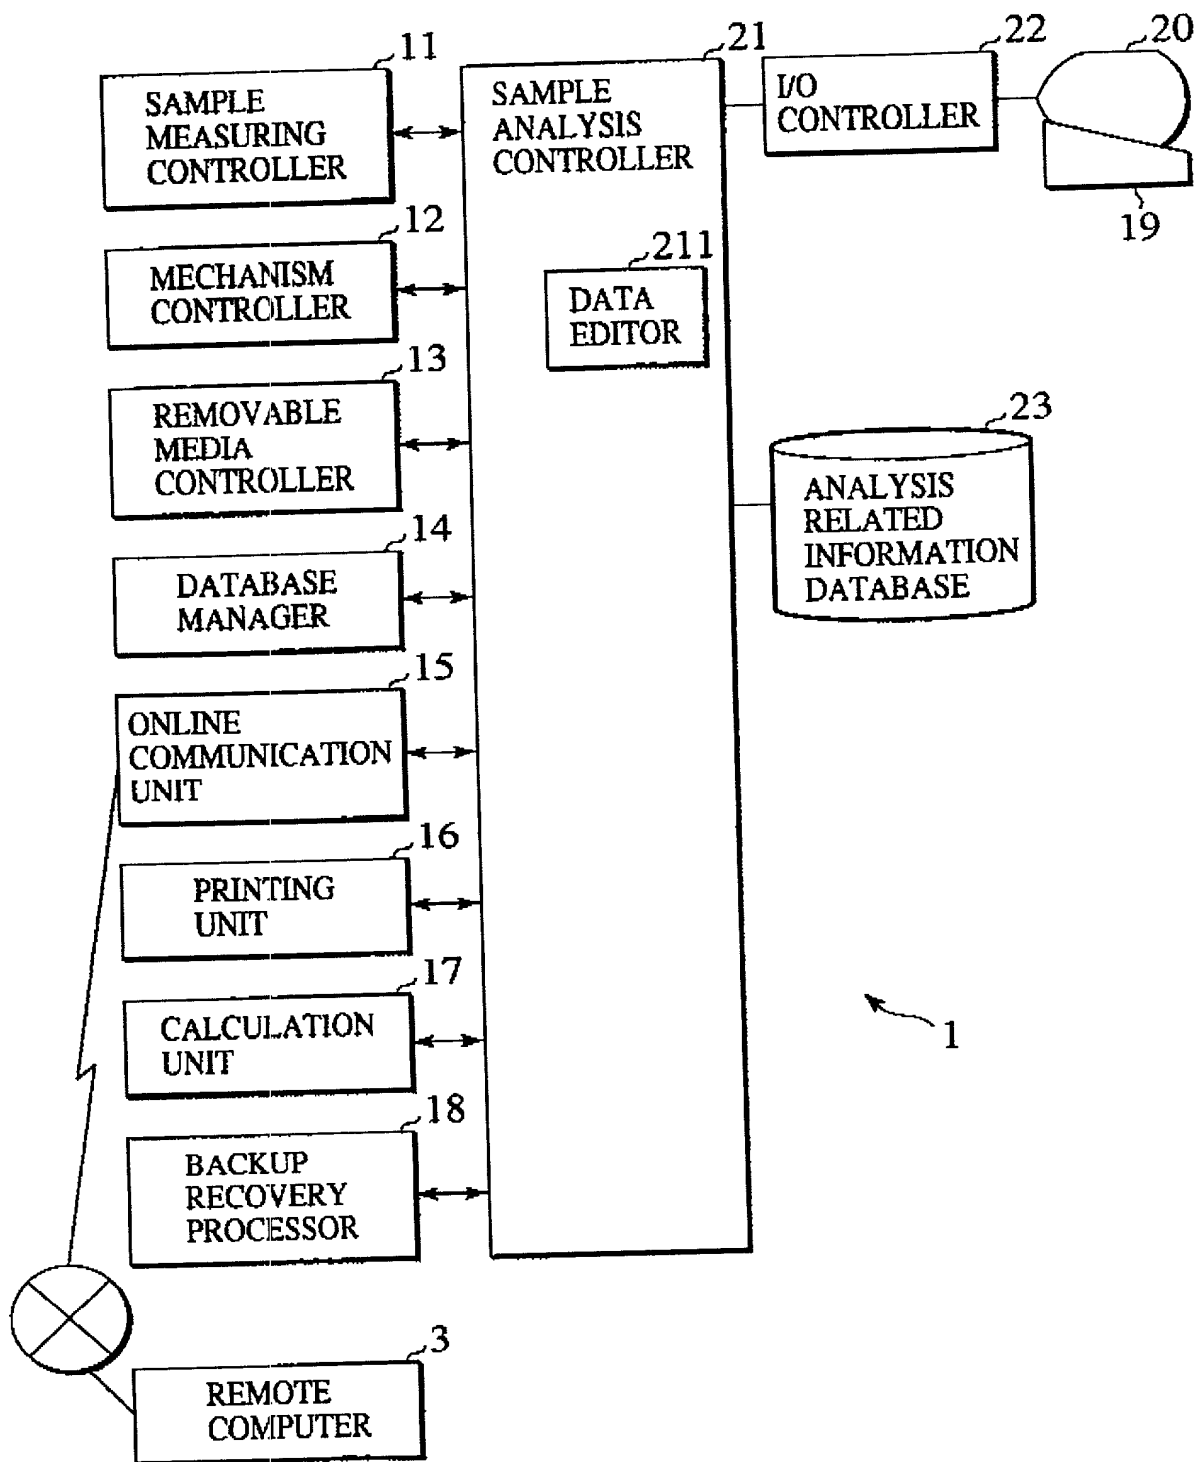


FIG.3


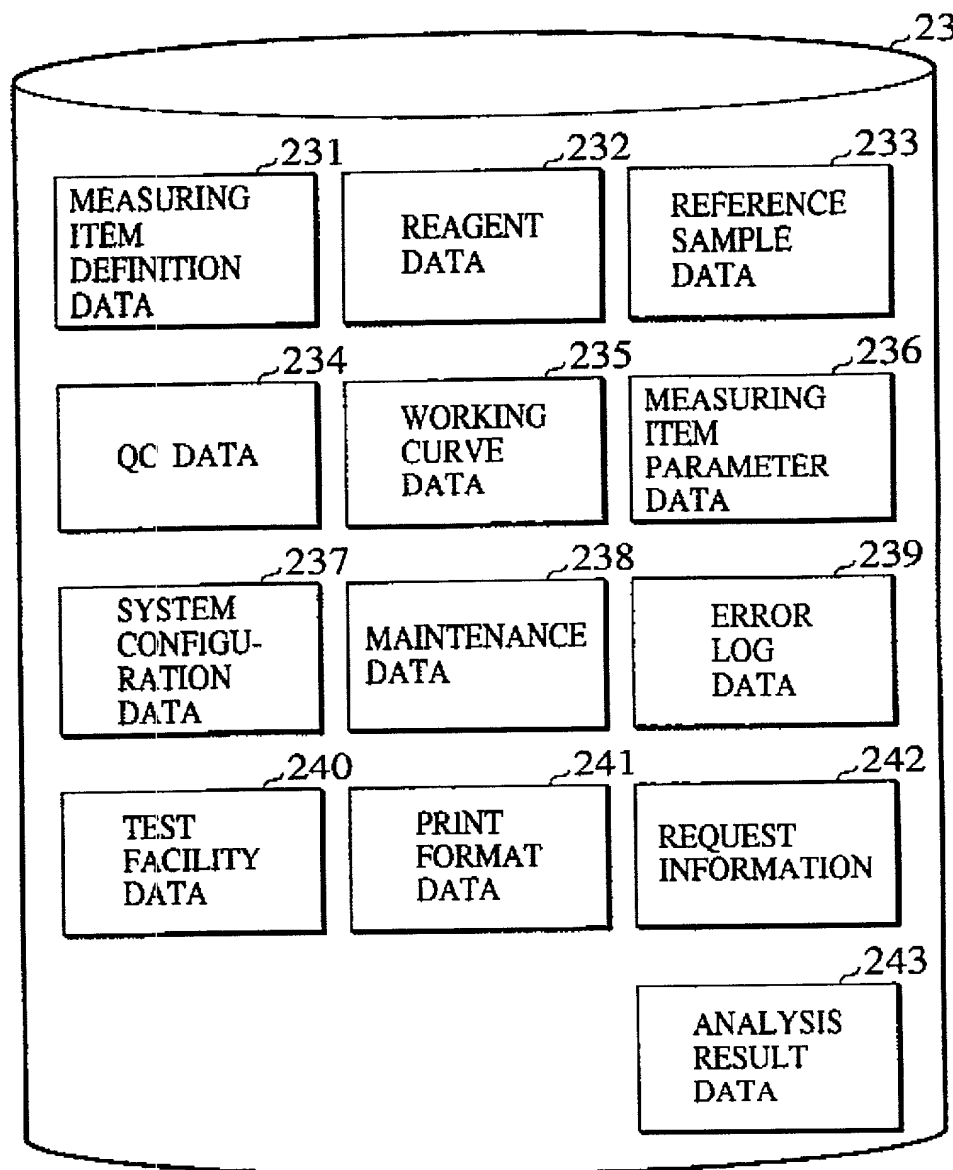


FIG.4

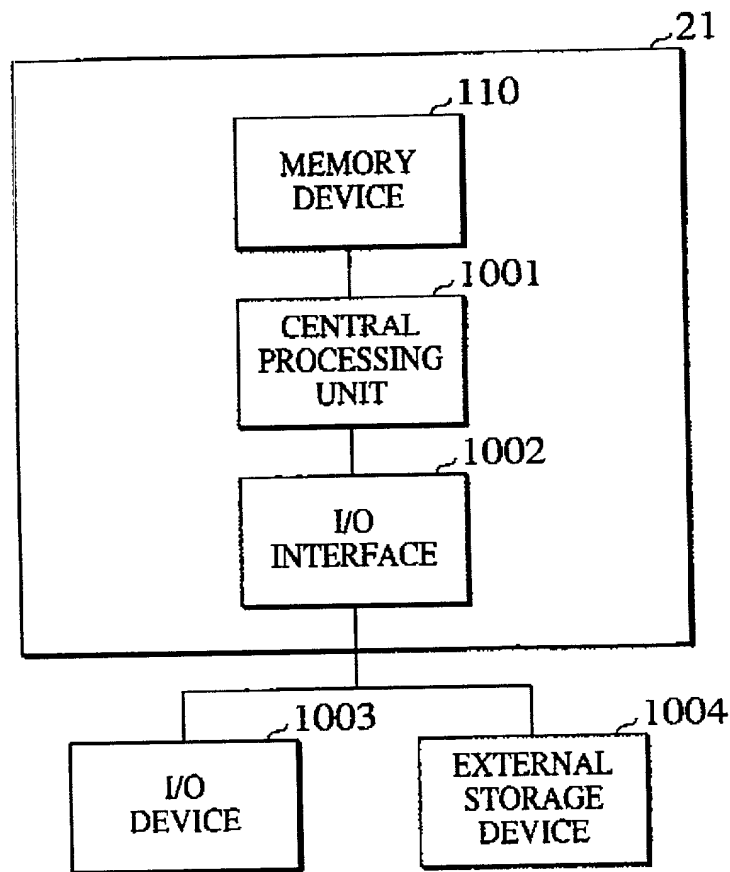

5/8

FIG.5

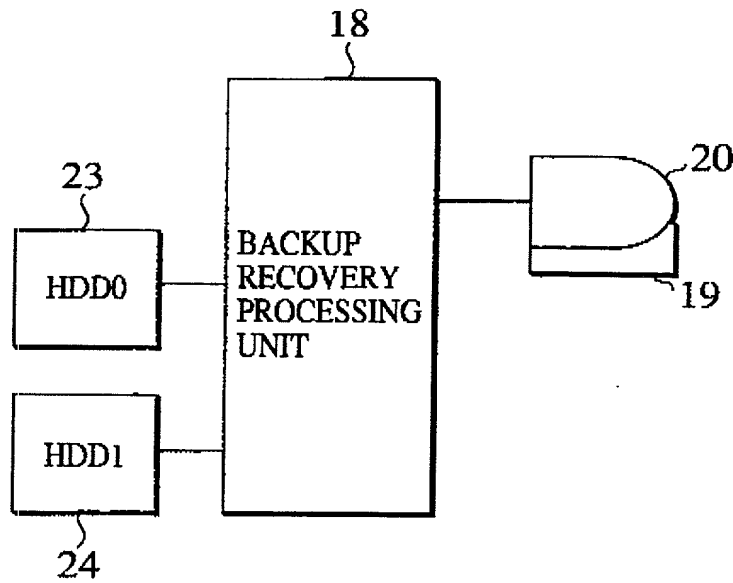


FIG.6

A screenshot of a graphical user interface window titled "BACKUP / RECOVERY". The window contains two main sections. The first section is titled "BACKUP" and contains a button labeled "BACKUP" followed by a checkbox and the text "ABOLISH PREVIOUSLY BACKED CONTENT". The second section is titled "RECOVERY" and contains a button labeled "RECOVERY" followed by a checkbox and the text "CORRESPOND TO ONLY A FILE IN USE". On the right side of the window, there are two buttons: "OK" and "CANCEL".

24

FIG.7

"REAGENT ID", "REAGENT NAME", "REAGENT TYPE",  
"BOTTLE TYPE", "LOT NUMBER", "EXPIRATION DATE"  
"99010001", "Ca", , 100, "0001", , "2000/1/1"

27

FIG.8

REAGENT INFORMATION LIBRARY		
REAGENT ID	<input type="text" value="99010001"/>	<input type="button" value="OK"/> <input type="button" value="CANCEL"/> <input type="button" value="LOAD"/> <input type="button" value="WRITE"/>
REAGENT NAME	<input type="text" value="Ca"/>	
REAGENT TYPE	<input type="text" value="R-1"/> ▾	
BOTTLE TYPE	<input type="text" value="100ml"/> ▾	
LOT NUMBER	<input type="text" value="00001"/>	
EXPIRATION DATE	<input type="text" value="2000/1/1"/>	

28

7/8

FIG.9

REAGENT DISPOSITION SETTING			
R1/R2	R1	R2	
POSITION	REAGENT NAME	REMAINING QUANTITY	▲
R1-1			
R1-2			
R1-3			
R1-4			
R1-5			
R2-1			
R2-2			
R2-3			
R2-4			
R2-5			▼

OK

CANCEL

SELECT

LIBRARY

29

FIG.10

```

<table>
  <column>
    <atrb>Reagent ID</atrb>
    <atrb>Reagent Name</atrb>
    <atrb>Reagent Type</atrb>
    <atrb>Cartridge Type</atrb>
    <atrb>Lot Number</atrb>
    <atrb>Expiration</atrb>
  </column>
  <item>
    <reagent ID>99010001</reagent ID>
    <name>Ca</name>
    <type>R-1</type>
    <cartridge>100</cartridge>
    <lot>0001</lot>
    <expiration>2000/1/1</expiration>
  </item>
</table>

```

30

FIG.11

